



ANALIZA BIAŁEK



100013459

## Laboratory of Analysis

**Client:** NOVAVITALITY  
**Order number:** 100013459  
**Name:** NOVAVITALITY.CO.UK BACTERIOSTATIC WATER  
**Number of samples:** 1 vial

**Batch number:** NV-260223-08  
**Recive date:** 2026-03-17  
**Start date:** 2026-03-19  
**End date:** 2026-04-02

### Sample identification


| Substance      | Method of taking a sample   | Form                               |
|----------------|-----------------------------|------------------------------------|
| Benzyl alcohol | Sample provided by customer | Transparent liquid in a glass vial |

### Results

| Substance      | Sample name                      | Content | Purity |
|----------------|----------------------------------|---------|--------|
| Benzyl alcohol | NOVAVITALITY.CO.UK BAC WATER 3ML | 0,95%   | -----  |

| Test                                     | Sample name                      | Result       |
|--|----------------------------------|--------------|
| TYMC                                     | NOVAVITALITY.CO.UK BAC WATER 3ML | PASS         |
| TAMC                                     | NOVAVITALITY.CO.UK BAC WATER 3ML | PASS         |
| Presence of presumptive Escherichia Coli | NOVAVITALITY.CO.UK BAC WATER 3ML | NOT DETECTED |
| Presence of Salmonella Spp.              | NOVAVITALITY.CO.UK BAC WATER 3ML | NOT DETECTED |

### Photo of the test sample

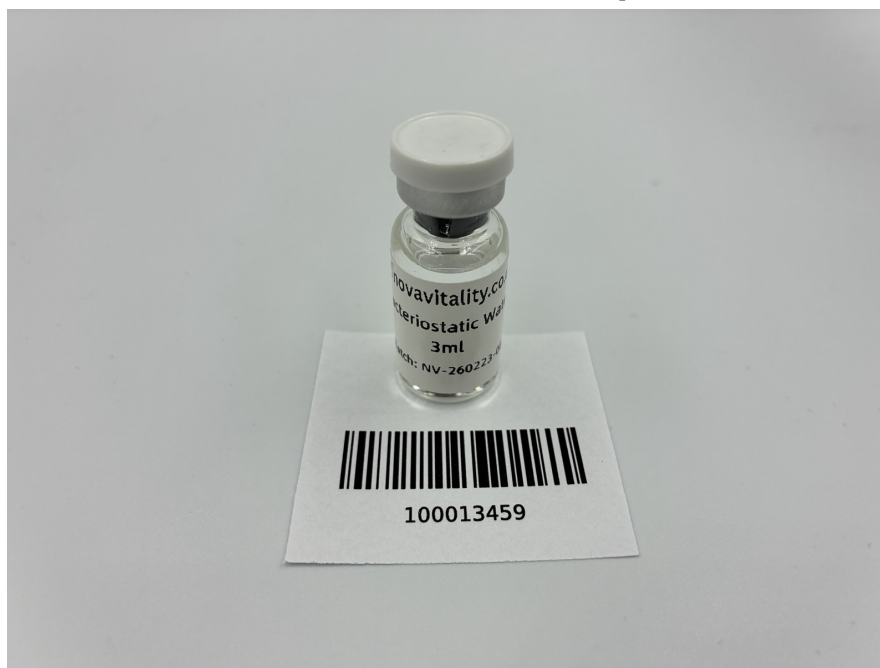

**Password**

45GP51SA

**Analiza Białek sp. z o.o.**  
**KRS:** 0000966168  
**NIP:** 8992922970  
**REGON:** 521751875

**Headquarters and Laboratory:**  
ul. Duńska 9, 54-427 Wrocław  
Budynek DELTA

**Lab technician:**  
Analysis and research specialist  
mgr Arkadiusz Zajęc